

# Certificate of Accreditation



## **Aerofin Laboratories Ltd**

Testing Laboratory No. 8408

**Is accredited in accordance with International Standard ISO/IEC 17025:2017  
– General Requirements for the competence of testing and calibration  
laboratories.**

This accreditation demonstrates technical competence for a defined scope specified in the schedule to this certificate, and the operation of a management system (refer joint ISO-ILAC-IAF Communiqué dated April 2017). The schedule to this certificate is an essential accreditation document and from time to time may be revised and reissued.

The most recent issue of the schedule of accreditation, which bears the same accreditation number as this certificate, is available from [www.ukas.com](http://www.ukas.com).

This accreditation is subject to continuing conformity with United Kingdom Accreditation Service requirements.

A handwritten signature in black ink, appearing to read "Matt Gantley", is positioned above a horizontal line.

**Matt Gantley**, *Chief Executive Officer*  
United Kingdom Accreditation Service

Initial Accreditation: 4 June 2015  
Certificate Issued: 25 January 2021



Scan QR Code to  
verify

## Laboratory Report

Date: 18th August 2023  
Report No. 48636 Revision 2

FUTURAL (UK) LTD  
128 City Road  
London  
United Kingdom  
EC1V 2NX

**Title: Corrosion Resistance.**

**Page 1 of 4**

**Part No:** Futural


**Material:** 3mm pre-coated aluminium

**Description:** 4000 Salt Spray & Adhesion - Pre-coated


**Customer Reference:** FUTURAL (UK) LTD

Date Received 01/03/2023


**Pre-coated  
Corrosion Resistance Testing iaw ASTM B117**

Panel ID	Result	Date and Stamp
1	Complete	16/08/2023 
2	Complete	
Tested in accordance with: AAMA2605-11 section 8.8.2		
Comments: Panels scribed in accordance with 8.8.2.1 of AAMA2605-11 prior to exposure. This activity is not covered by the UKAS scope. 4000 hours exposure at 20° to the vertical		

**Performance: Rating of failure at scribe.**


Panel ID	Result	Date and Stamp
1	Rating 10 (Top rating) - Pass	18/08/2023 
2	Rating 10 (Top rating) - Pass	
Tested in accordance with: AAMA2605-11 section 8.8.2.2		
Comments: Method of paint removal: tape removal in accordance with para 8.8.2.1 of AAMA2605-11.  This activity is not covered by the UKAS scope.		

**Performance: Rating of un-scribed areas.**

Panel ID	Result	Date and Stamp
1	Rating 10 (Top rating) - Pass	18/08/2023 
2	Rating 10 (Top rating) - Pass	
Tested in accordance with: AAMA2605-11 section 8.8.2.2		
Comments: Method of paint removal: tape removal in accordance with para 8.8.2.1 of AAMA2605-11.  This activity is not covered by the UKAS scope.		



Post exposure, post tape removal.

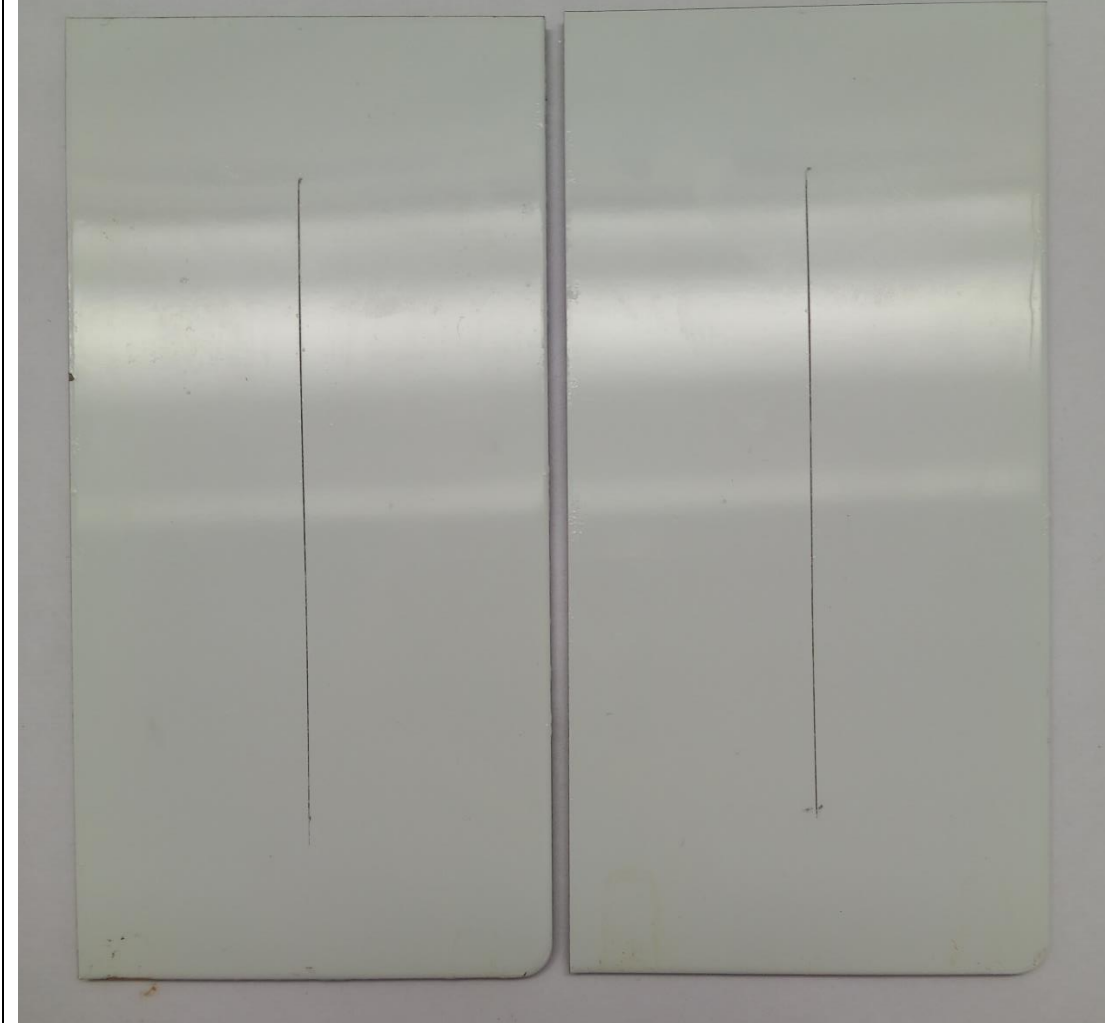

The above test results relate only to the sample as received.  
Testing is performed at ambient temperature unless otherwise stated in the report.  
Operators performing analysis have been appropriately trained and training records are available upon request.  
A full list of apparatus used and the calibration details are available upon request.

This report shall not be reproduced except in full without the approval of Aerofin Laboratories Ltd

**Key technical signatory:****N.Sverdloff - Principal Scientist - Chemistry Lead****Test report approved by:****M.Machnowska – Principal Scientist – Quality Lead****A.French – Operations Director****In accordance with AMP 7.8 para 3.3.1 j & para 3.7**

---

END OF TEST REPORT